


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument


State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program JUL 09 2009


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130570
Name		STEVE DUNN	ID# 4106 Date 7-9-09
A	Agency	APD	Phone # 786-8900
Instrument Location		4 th AVE SUB.	
Alco S/N		78895	Target Value .084 High Pressure 500 PSI
B	Alco Test Value Average		.076 1 st Alco .077 2 nd Alco
Signature		 7/14/09	
(OVER)			


I, Nita J. Bolz, after being first duly sworn, depose and state as follows. (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.

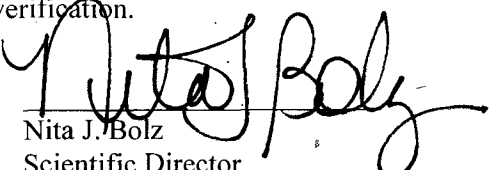
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 2nd day of Jul, 2009.

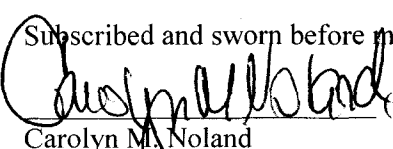
(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office.



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130570

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

S. DUNN #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130570

JULY 09, 2009

OPERATOR'S NAME:

DUNN/S

OPERATOR'S NUMBER: 4106

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

V

O.L. #: V

DEPT/AGENCY: AHC1

CASE/REPORT: V

TEST TYPE: V

ALCO TARGET VALUE: .004

ALCO S/N: 78895

--- BREATH ANALYSIS ---

.004 ADJUSTED FOR 30.19 in

ALCO TARGET .004 04:56

BLANK TEST .000 04:57

INTERNAL STANDARD VERIFIED 04:57

ALCO TV 30.19 in .076 04:57

BLANK TEST .000 04:58

SUBJECT SAMPLE .000 04:58

BLANK TEST .000 04:59

ALCO TV 30.19 in .077 04:59

BLANK TEST .000 05:00

DIAGNOSTIC CHECK

S. DUNN #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130570

JULY 09, 2009

TIME 04:54

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 12/11/08

HEATERS

SAMPLE CHAMBER: 52c

BREATH TUBE: 42c

BAROMETER: 30.19 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!""%&'()*+,-./0123456789:;<=>?@ABCDEFGHI
HIJKLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~